SmartVS version 1.09.00 - Software Update 2022-10-03

Dear SmartVS Users,

A new version of SmartVS has been released. In this version we have the following new features:

The StimGen application can be accessed from the SmartVS Launchpad control panel without the need of a password:

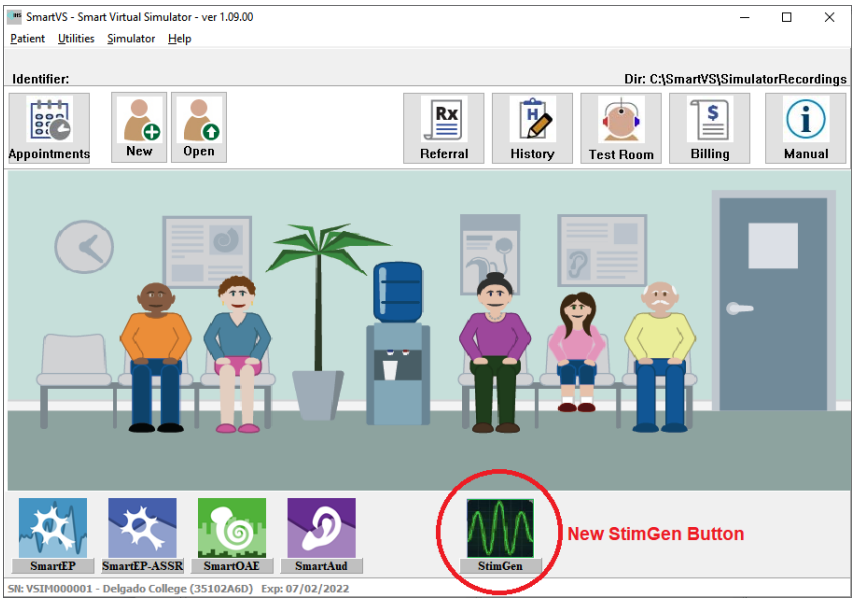

Easy to access wave parameters will allow students to add and edit component characteristics to learn how signal harmonics come together to generate more complex signals such as triangular waveforms.

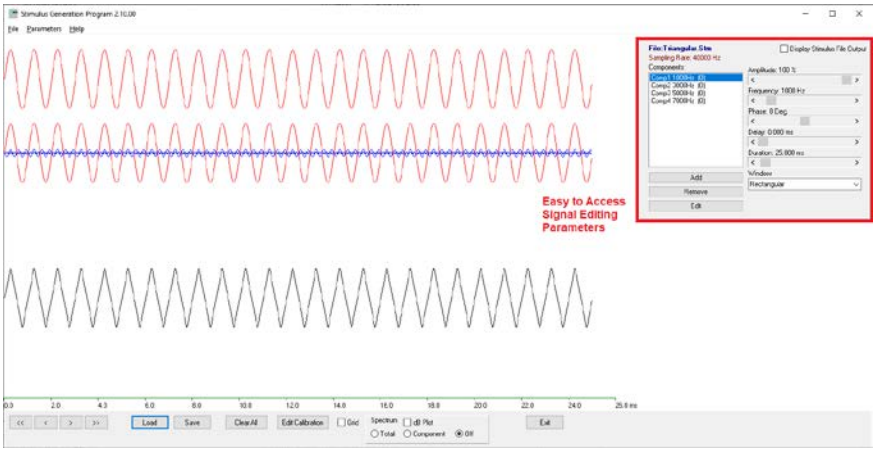

The audiometer module will display a Feedback button for Practice Patients, so students can see how well their audiogram matches the patient's true programmed audiogram.

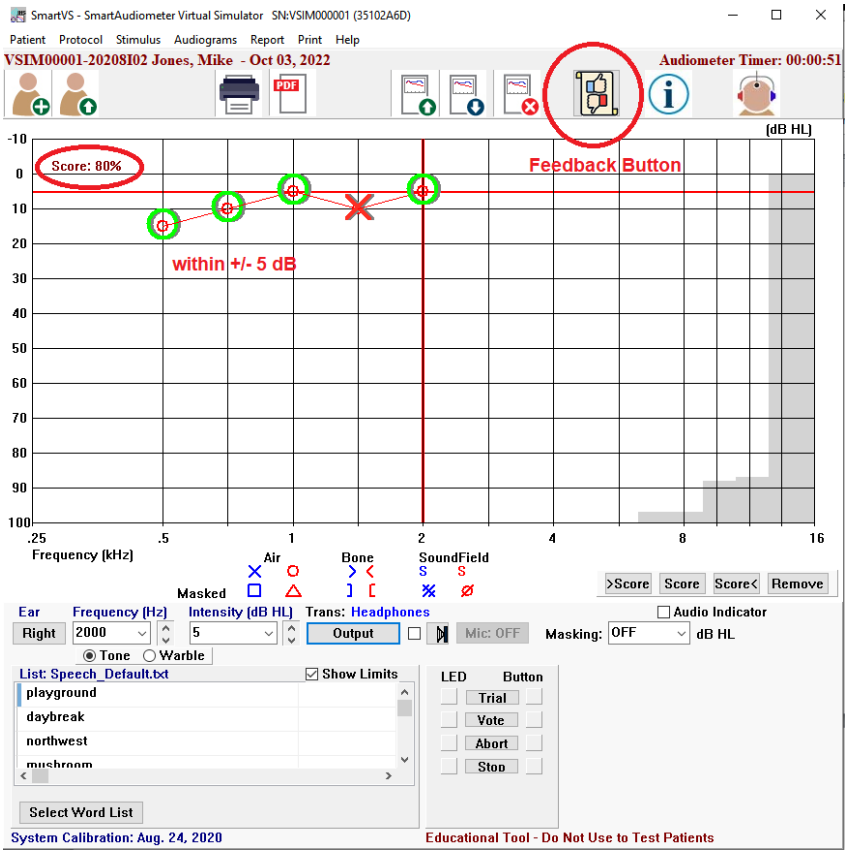

The Word Recognition Score (WRS) now incorporates a correct response probability based on the testing intensity.

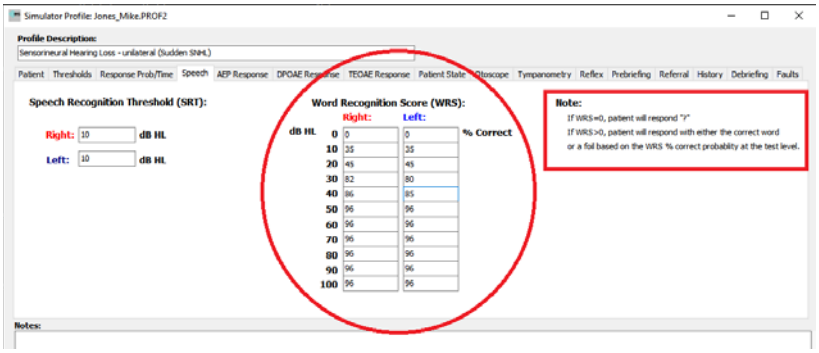

From the Test Room – Students can practice giving oral instructions to patients. They can record and play back the instructions for feedback from their instructors.

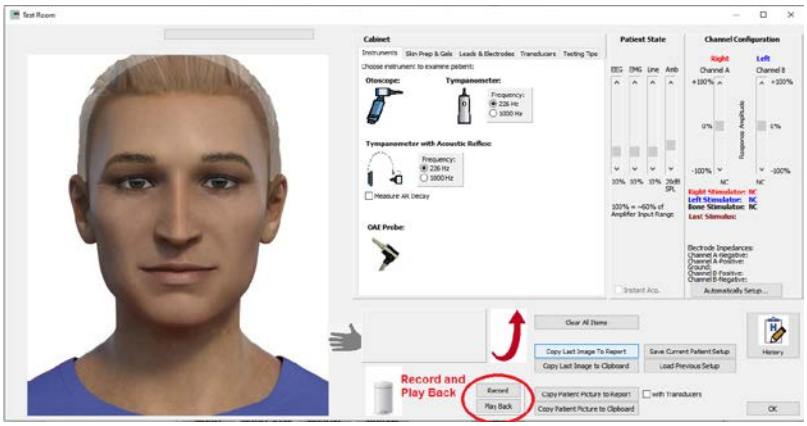

We are currently working on developing new patients. These will be released very soon!

Please note that the update name is **SmartVS109.DAT**. This update will download the latest version of the software and recently modified patient profiles.

To download these updates, please follow these instructions:

1) First launch the Updates utility from you Help menu in the SmartVS waiting room:

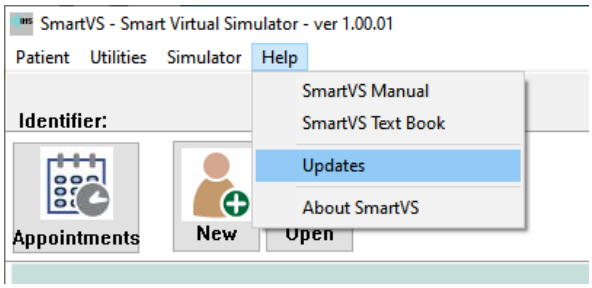

2) When the update program launches, type the update name in the Update Name edit box as shown below:

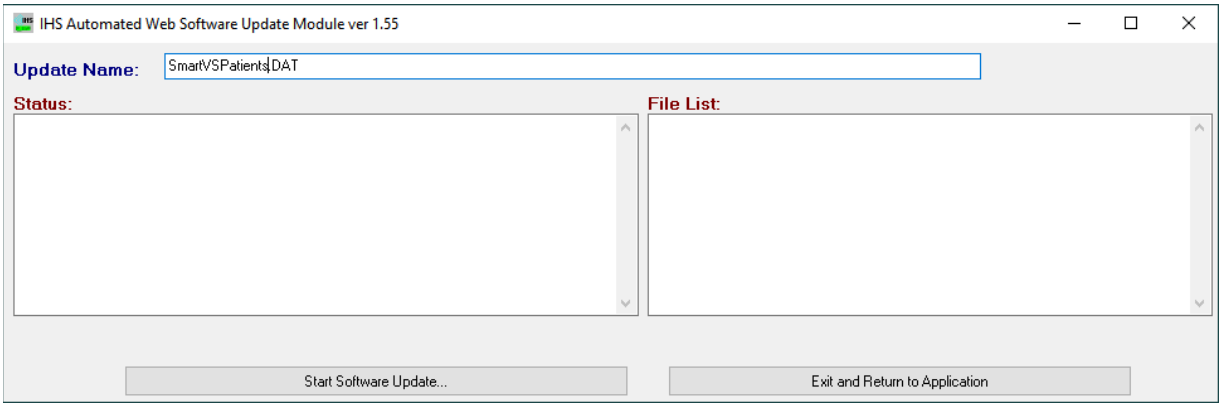

You will need to run the following update:

3) Type SmartVS109.DAT to update your SmartVS software.

After entering the update name, press the **[Start Software Update]** button. When completed, you will see a **"Finished"** message box displayed.

If you have previously run this update, you will see the following message:

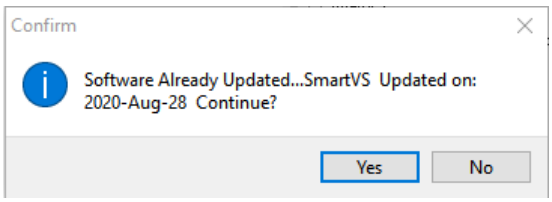

Just press the [Yes] button to continue with this new update.

4) After running the updates, press the **[Exit and Return to Application]** button to launch SmartVS again.

If you have any questions, please contact us at **SmartVSSupport@ihsys.com**

News for Apple Mac Users

We have tested SmartVS on Apple Mac computers using PlayOnMac and all features work great! Just make sure you have MacOS Catalina (10.14) or Higher (11.x) and a SmartVS Web license. If you currently have a dongle license and would like to obtain a web license to use on your Mac, please contact IHS. You can install PlayOnMac from the following link: https://www.playonmac.com

News for ISAO Users

The new version of the IHSSimulator software will also be released in July. Now you can use all your SmartVS profiles on the IHS ISAO Simulator! Student will now be able to practice at home using SmartVS and record from the same patient profiles in the lab using actual testing equipment connected to the simulator.